


Edit Calibration

Result: Qualitex 31-03-09

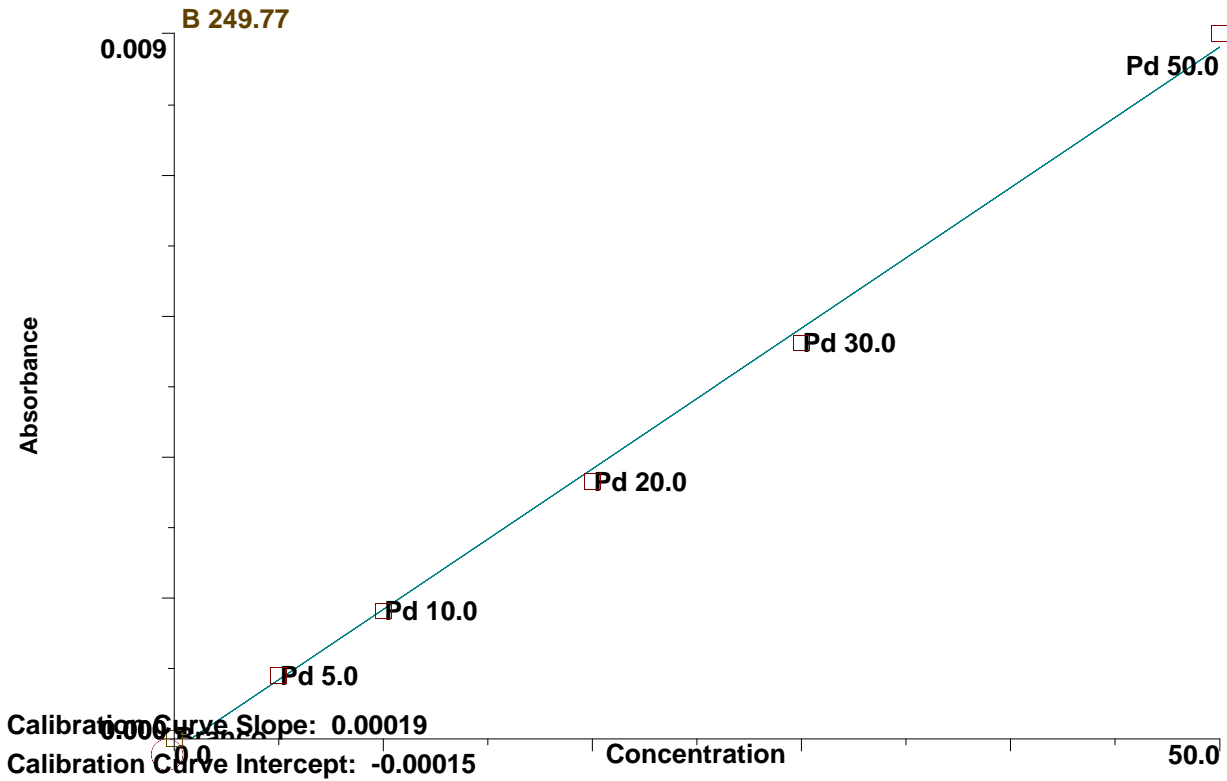

Calibration Curve Slope: 0.00019
 Calibration Curve Intercept: -0.00015
 Calibration Curve Correlation Coefficient: 0.998969
 Calibration Curve Type: Linear, Calculated Intercept
 Current Sample Concentration: -0.339 mg/L

Std #	Standard ID	Entered Conc.	Calculated Conc.	Action
Blank	Branco	0	0.784	Include
1	Pd 5.0	5.0	5.293	Include
2	Pd 10.0	10.0	9.879	Include
3	Pd 20.0	20.0	19.112	Include
4	Pd 30.0	30.0	28.954	Include
5	Pd 50.0	50.0	50.978	Include
31/03/09 12:53:38				